


Centrifuge Tubes


Centrifuge Tubes and Stand

Centrifuge Tubes are used to monitor the concentration of magnetic particles and the level of contamination in a fluorescent and non-fluorescent bath.


Part Number	Description	Measurements
MG10T	General Centrifuge Tube	1.5 ml with .05 ml graduations
MG10TF-C*	Certified Fluorescent Centrifuge Tube	1 ml with .05 ml graduations
MG10TNF-C*	Certified Non-Fluorescent Centrifuge Tube	1.5 ml with .1 ml graduations
MG10S	Centrifuge Tube Stand Only	-

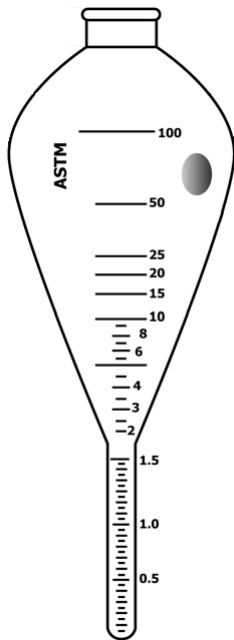


MG10T

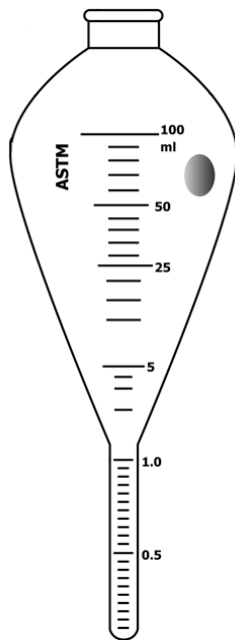

MG10TF-C

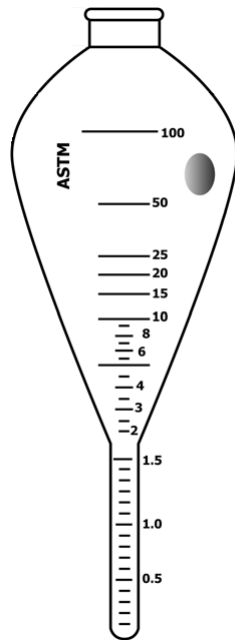

MG10TNF-C

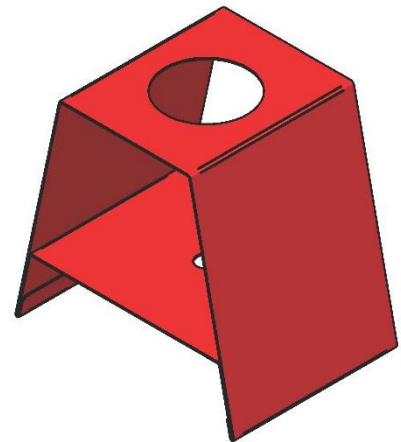

MG10S

*Standard Compliance: ASTM E709