



**OPERATING INSTRUCTIONS
MODEL BAC310
AC POWER SUPPLY**

**BULLETIN 255-1
Dec. 2023**


PARKER RESEARCH CORP.


NONDESTRUCTIVE TEST METHODS, SYSTEMS, INSTRUMENTS
BOX 1406, DUNEDIN, FLORIDA, U.S.A. 34697
PHONE: (727)796-4066 FAX: (727)797-3941

INSTRUMENT DESCRIPTION: The BAC310 battery operated Inverter Power Supply is a totally portable, stand-alone power source. It is designed to operate the Parker 100, 300 and A410 series 115VAC, AC Yokes (Contour Probes).

The BAC310 operates independently from any outside power source. Power is derived from the internal 12VDC battery, which is inverted to 115VAC output through the inverter circuitry. A separate battery charger is provided for overnight charging of the battery. The entire BAC310 unit is contained within a heavy-duty steel case 13-1/4" H X 10-3/4" W X 7-1/4" D and weighs only 30 pounds. The BAC310 may be used in a shop or field applications (away from water) and is ideal in areas where normal AC line power is unavailable or where outside power sources may present a safety concern.

SAFETY PRECAUTIONS: The BAC310 is a high voltage (115VAC) electrical device. Care should be taken to avoid electrical shock. Read all directions and safety precautions thoroughly before using. Do not use this equipment in or near water. Avoid exposure to rain.

 **DO NOT** attempt to operate other electrical devices from the BAC310. It is designed to power the Parker B100, B300, A410. **Note:** The BAC310 will not operate the DC mode of AC/DC Yokes.


 **DO NOT** attempt to operate more than one Yoke at the same time. The BAC310 is designed for operation of one instrument at a time only.

A.C. YOKE OPERATION: The BAC310 will operate the Parker B100, B300 or A410 AC Contour Probes (Yokes). With a fully charged battery, plug the standard plug of the Yoke into one of the output sockets. Toggle the ON-OFF switch to the ON position. There is nothing else to do. The Contour probes will function normally. Verify that the Probe will comply with the 10-pound weight lift test before and during use. Follow the operating instructions for the Yoke for correct and normal AC Yoke inspection techniques and requirements. A slight pulsing of the Probe may be felt. This is a characteristic of the inverter circuitry and has no effect on the normal operation of the Probes. The Parker B100, B300 and A410 will exceed applicable standards requirements.

BATTERY: The battery contained within the BAC310 is a sealed, lead acid type rated at 20Ah, 12VDC (**Figure 2, Item 1**). The battery will provide power to operate the Parker B100, B300, and A410 for approximately two hours under normal conditions. Extended "time-on" of the Yokes will reduce this time. When battery level becomes too low for operation, the unit will shut down. The battery must then be recharged (overnight) or replaced by the optional BAC60-60 battery pack.

BATTERY CHARGING: When it becomes necessary to recharge the battery, the BC310 battery charger is provided (**Figure 2, Item 2**). This is a trickle type charger rated at 12VDC, 1.5 amps allowing for overnight charging.

Open the BAC310 case cover and remove the charger. Plug the battery charger connector into the connector of the battery. These will only connect one way. The exposed metal pin is the Ground. Plug the battery charger into a standard 115V outlet.

 **CAUTION:** The BAC310 cover should never be closed during battery charging. Always charge the battery in a well-ventilated area. Always disconnect the AC power cord before connecting or disconnecting the charger from the battery. **ALWAYS WEAR EYE PROTECTION WHEN CHARGING OR REPLACING THE BATTERY.**


BATTERY REPLACEMENT: The battery pack contained within the BAC310 may be changed to extend operating times. To replace the battery pack, disconnect the inverter plug from the battery socket. Remove the two battery bracket screws located on the rear of the steel case (**Figure 2, Item 3**). Lift the entire battery and bracket assembly straight up and out of the case with one finger placed through bracket hole (**Figure 2, Item 4**). Replace it with the optional BAC60-60 replacement battery pack. (Be sure it is fully charged). Lower the entire battery pack assembly into the case. Align the holes of the battery bracket screws. Replace and retighten the screws. Connect the inverter plug into the battery pack socket.

BATTERY DISPOSAL: Always dispose of batteries according to the requirements of local ordinances. Follow all cautions on the battery.



ALWAYS WEAR EYE PROTECTION WHEN WORKING WITH THE BATTERY.

FUSE: The BAC310 battery is fused with an in line 35A Maxi style fuse (**Figure 2, Item 5**). In the event the unit fails to function, check the fuse, and replace if necessary.

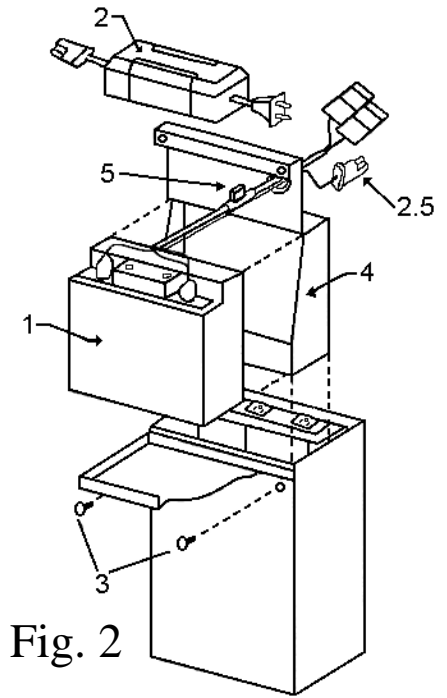

Parker Research – 90 Day Warranty

The BAC310 is warranted against malfunction due to defective material and workmanship. The defective unit will be repaired or replaced (less incoming freight charges) for a period of 90 days from the date of sale. The warranty will not apply to units that have been altered or to those units that have been used improperly. The warranty will not cover damage to other devices that have been plugged into the BAC310. Repair or replacement of the defective unit will be made at the discretion of Parker Research Corporation. The repaired or replacement unit will be returned to the original customer prepaid.

The obligation of Parker Research Corporation is limited to the repair or replacement of the defective unit. No other obligation is expressed or implied. Parker Research Corporation assumes no liability from any claim arising from the use of this equipment.

CAUTION: For the correct and safe use of this equipment, training of operating personnel is required. Use of proper inspection procedures, standards compliance and safety requirements is the obligation of the user.

ALWAYS WEAR EYE PROTECTION WHEN USING THE EQUIPMENT.

**PARKER RESEARCH CORP.
2642 ENTERPRISE ROAD WEST
CLEARWATER, FL 33763**